Proceedings of the International Symposium on Biometrics and Security Technologies (IEEE ISBAST 2008*)*, Bahria University, Islamabad, Pakistan, April 23, 24, 2008, IEEE Catalog Number: CFP0859D, Digital Object Identifier: 10.1109/ISBAST.2008.4547657, Date Published in Issue: 2008-06-20 14:11:26.0, ISBN: 978-1-4244-2427-6, Library of Congress: 2008903490

Pattern Recognition using Moiré Fringe Topography and Rasterstereography

Syed Arif Kamal*
University of Karachi, Karachi, Pakistan

Abstract– Moiré fringe topography and rasterstereography are 3-D optical imaging techniques, which provide height and curvature maps of the subject or the object under study. These are non-contact and non-invasive techniques, which project moiré and raster grids on the body. The distorted grids contain height and curvature information, which may be recovered using image-processing algorithms. These techniques are being applied to face recognition. The information may be stored in the database and not easily accessi-ble to ordinary citizen. Hence, the chances of fake pictures or fabricated patterns are mini-mized. Techniques are developed to project, simultaneously, moiré and raster grids and analyze height and curvature information, separately, using selective optical filtering, which could be used to record height and curvature patterns during a certain action, *e. g.*, uttering a standard word. Edge-based algorithms, combined with moiré contours and raster patterns, allow study of face move-ments through changing height and curvature maps. A multiple-level screening of suspects using these technologies is proposed.

Keywords–Face recognition, stereophotography, image processing

I. Introduction

There is a need for security systems, which do not violate subject's privacy, have high sensit-ivity (very few or no missed cases) as well as high specificity (very few or no false positives) and avoid human exposure to harmful radiation. Photrogrammetry has come up with the solution. Being non-invasive, non-contact and non-disruptive technique, it avoids risks involved in hurting, infecting or distorting the human subject being studied. Photogrammetry can make it easy to measure objects otherwise inaccessible or difficult to measure and has the capability to either discard images or provide permanent record. Any desired degree of accuracy may be achieved by making a suitable choice of equipment and technique. Data obtained from photogrammetric measurements, especially if put in coördinate form, may be easily utilized by computer systems [1].

The different photogrammetric systems, which could be employed in security technologies, are stereophotography, holography, thermography, 3-D video laser scanning, edge-based and intensity-based algorithms, moiré fringe topography [2-4], rasterstereography [5, 6] and edge-based moiré [7]. This paper deals with the application of last three techniques and introduces edge-based raster as well as a multi-level screen-ing of suspects. The checks located at the top level are designed to be highly sensitive. The checks located at the bottom level are chosen to be highly specific. The same concept was used in the multi-level screening proposed for scoliosis [8].

II. 3-D Imaging Techniques: Systems

In this section, systems for moiré fringe topography, rastersterography, simultaneous moiré and raster recording, edge-based moiré and edge-based raster are discussed:

A. Moiré-Fringe Topography

Moiré fringe topography provides a 3-dimensional height map of the human face without using X rays or any other ionizing radiation harmful for human beings [9-11] and can be handled using various algorithms [12]. Moiré fringes are a series of interference fringes arising from the superposition of sets of parallel lines or threads, the sets being slightly inclined to one another. Width of the grid lines should be equal to the space between them. It has been applied in the detection [8, 13-18],

*Convener, National Curriculum Revision Committee (Mathematics), Higher Education Commission; Professor, Department of Mathematics, Interdepartmental Faculty, Departments of Computer Science, Chemistry and Physics, University of Karachi; *paper mail*: University of Karachi, Box 8406, Karachi 75270 (Pakistan); *e-mail*: sakamal@uok.edu.pk; *homepage*: http://ngds-ku.org/kamal
Member AIAA, IBRO

1-4244-2427-6/08/$20.00 ©2008 IEEE

the documentation [19-21], the quantification [22-27] and the follow up [28] of trunk deformities, posture [29] and gait analysis [5, 6, 30] as well as study of neurological disorders [31, 32]. Various forms of moiré systems are described below:

i) Basic Form or Shadow Type Moiré: The shadow type moiré fringe topography apparatus [33] in use in Karachi consisted of a lightweight wooden frame of external dimensions 57 x 133 cm (grid 52 x 108 cm). Black nylon fishing line of diameter 0.85 mm was wound vertically using a spring of pitch 0.75 mm. Special reinforcement techniques are needed to prevent breaking of frame from thread tension. This method is simple and gives a lot of information, but it requires a large scale of equipment and it is difficult to maintain the standard of human bodies. In Malmö, Sweden the author worked on a moiré system, in which the moiré grid was sandwiched between two glass panes.

ii) Projection Type Moiré: In projection type moiré-fringe topography the human body is supported on a standard holder and a grid image is projected on the face to form a transformed image according to shape of the face. This image shall, then, be formed on a standard grid through a lens so as to generate contour line moiré fringe by superposing the transformed grid on the face. This method gives a large amount of information. Accuracy can be changed by changing grids.

In both the shadow and the projection type, the fringes are visible to the naked eye and, hence, can be used in setups, where a permanent record in the form of a photograph is not required. The fringes could also be recorded on videotape. However, mis-positioning cannot be corrected after the picture is recorded.

iii) Grating Hologram Type Moiré: Grating hologram type moiré fringe topography has the capability of adjus-ting the moiré fringes after recording. Grating hologram type of system consists of projecting a moiré grid (Fig. 1) on a child's back and photographing the distorted grid. The reference grid is re-projected at the same angle and with the same magnification on the photograph of the distorted grid to view moiré fringes. For gait analysis and simultaneous moiré and raster recording, grating-hologram type was found to be most suitable.

B. Rasterstereography

Rastersterography is very similar to stereophotography. Difference is that one of the cameras is replaced by a slide projector projecting a raster (Fig. 1*b*) on the face [5, 6]. Because of the curvature of the body the raster is distorted. Study of this distortion provides information about the topological properties of the surface under study. The remarkable feature of rasterstereography is that it does not require a specific arrangement of apparatus to obtain meaningful rasters, whereas only a specific geometry of the moiré set up would provide contours with the desired mathematical properties.

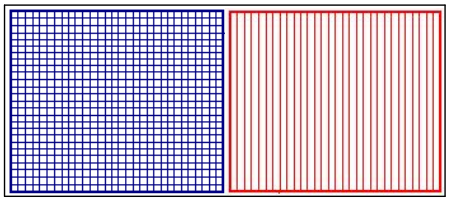

Fig. 1*a*, *b*. Grids for rasterstereography and moiré fringe topography (right)

C. Simultaneous Moiré and Raster Recording

For simultaneous moiré and raster recordings our group used a camera, 2 projectors, a raster grid and a moiré grid (Fig. 1) [6]. Moiré grid was prepared in red color and raster grid prepared in blue color. Both the grids were simultaneously projected on the body using two projectors as shown in Fig. 2. After a color photograph was obtained, a red filter matching with the color of the original moiré grid was placed on it. The red moiré grid became invisible and the blue raster grid appeared black. These were, then, fed in the scanner for analysis using rasterstereography algorithms. Similarly, a blue filter matching with the color of the raster grid was placed on the picture. Raster was suppressed and the moiré grid appeared black. Then a standard moiré grid was projected at the same angle to produce moiré fringes. Success of this procedure depends, critically, on proper matching of the colors.

D. Edge-Based Moiré

This is a combination of edge-based algorithm and moiré pattern [7]. Since moiré contours provide height maps in a plane perpendicular to the image, moiré patterns would change if the object is performing infinitesimal movements towards or away from the observer. Consider moiré patterns of face of a person. If that person starts speaking, the moiré patterns would, also, move. If the person's lips are moving away from the observer (lips are convex surfaces) the patterns would start converging and appear to sink. Movement away from the observer, therefore, corresponds to a sink field in the moiré patterns of the convex surface (Fig. 3a)

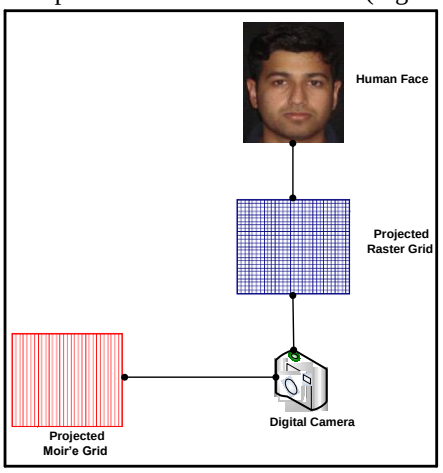

Fig. 2. Layout for simultaneous moiré and raster recording

1-4244-2427-6/08/$20.00 ©2008 IEEE

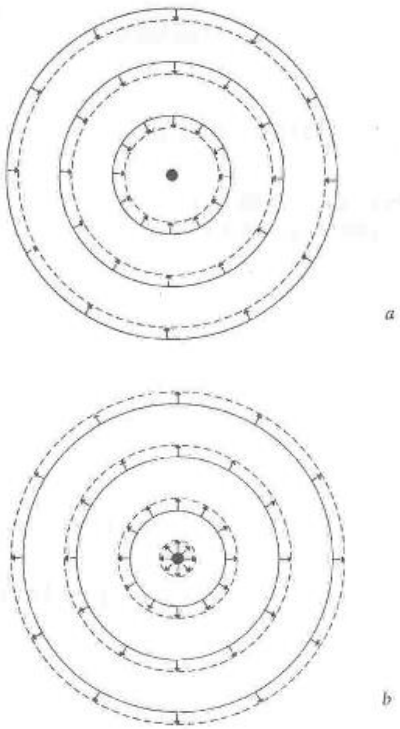

Fig. 3*a*, *b*. *Edge-based moiré* for movement normal to plane of paper for a convex object (top picture) object receding from the observer and object coming towards the observer

When the person's lips are moving towards the observer, new diverging patterns would appear (Fig. 3b). Movement towards the observer, therefore, corresponds to a source field in the moiré patterns of a convex surface.

E. Edge-Based Raster

This is a combination of edge-based algorithm and raster pattern. Since raster contours provide curvature maps, raster patterns would change if the object were performing infinitesimal movements towards or away from the observer. Consider raster patterns of face of a person. If that person starts speaking, the raster patterns would, also, change. The new and the old patterns could be connected by edge-based algorithm and curvature change could be represented as a vector field.

III. 3-D IMAGING TECHNIQUES: PARAMETERS FOR STUDY

In order that the information obtained from these photogrammetric techniques is scientifically relevant, one must consider the following**:**

A. Image quality

Image quality depends on a number of factors. Some of the considerations are**:**

i) Sharpness of Image: To obtain sharper fringes for our fishing line shadow type moiré system we used parallel light from a slide projector and applied talcum powder on child's back. Image quality depends critically on the choice of light source. Our group is in the process of evaluating fringe quality using torchlight, gaslight, candlelight and collimated candlelight.

ii) Distortions: The more are the optical elements in the system the more is the distortion. Therefore, one would realize that as compared to shadow type the distortion error in projection type and grating hologram type is a factor of 2-3 in the depth and in the sides. Distortions in our grating hologram type system have been minimized.

B. Reproducibility

Our group found the moiré technique to be 99.5% reproducible [34, 35]. Tests were conducted using Swedish system (pitch 2 *mm*) with moiré grid sandwiched between two glass panes.

C. Accuracy and Precision

There has been an interest in accuracy analysis of moiré systems used in scoliosis screening [36, 37]. Accuracy and precision of our fishing-line-shadow system (pitch 1.5 *mm*) have been estimated as 99.61% and 91.21%, respectively [38].

D. Sensitivity and Specificity

99.7% sensitivity of moiré fringe topography is reported in the literature in the context of scoliosis screening [39]. However, sometimes because of mis-positioning subjects a large number of false positives are generated [13]. To reduce these false positives (that is, increase specificity of moiré) we took moiré topographs on a level surface [8, 16], sometimes used an alignment system [40] and corrected leg-length inequalities. Further, referrals were based on more than one test and not on a single test. Similar criteria need to be established for face-recognition algori-thms.

IV. A MULTI-LEVEL SCREENING SYSTEM TO ESTABLISH IDENTITY

To establish identity with a high level of sensitivity and specificity, the following system is proposed**:**

Level 1: Height + Blood Group + 2-D Face Photographs (frontal plane and sagittal plane), without glasses, ear(s) exposed (high sensitivity)

Level 2: 3-D-Height and -Curvature Maps (frontal plane and sagittal plane), using moiré fringe topography and rasterstereography (Fig. 4), subject silent

Level 3: 3-D-Height and -Curvature-Video Clip (frontal plane and sagittal plane), using moiré fringe

topography and rasterstereography, subject uttering a standard sentence (high specificity)

Once the algorithms are developed, the system could be used to store data on a mega scale. The parameter, height, at the initial level is applicable to individuals, who have reached their peak height, *i. e.*, boys after the age of 21 years and girls after the age of 19 years.

V. Conclusion

Pattern recognition using moiré fringe topography and rasterstereography is expected to become a useful tool in security technologies. These techniques may find immediate applications in computerized re-construction of faces and patterns. Unlike holography moiré and raster techniques do not require the subject (or object) to be still. Hence, these techniques are ideal to describe infinitesimal motion of lips. In case, the visible pattern of face is altered due to plastic surgery, burn or accident, the motion of lips may, still, have signatures for identification. An immediate visual illustration of the magnitude and the direction of motion is available by combining edge-based algorithm with moiré contours. Edge-based moiré, therefore, makes it possible to have a three-dimensional map (position) and a three-dimensional motion profile (velocity) without involving differentiation. The moiré technique combined with rasterstereography may prove to be useful in providing non-contact, non-destructive, non-invasive, safe and reliable methods to study face patterns. Computations may be simplified using multi-grid techniques [41].

There is, however, a need to determine sensitivity, specificity, accuracy, precision and reproducibility of all the tests involved in a multi-level screening procedure. A comprehensive statistical model representing sensitivity and specificity of combination of tests used at a certain level is desirable. For the test to be universally acceptable, combined sensitivity of the top-level-screening module should exceed 95%, and the combined specificity of the bottom-level-screening module should not be less than 95%.

Moiré fringe topography and rastersterography have been applied in the study of posture and gait of children. A future screening system should combine posture and gait analysis with changing face patterns.

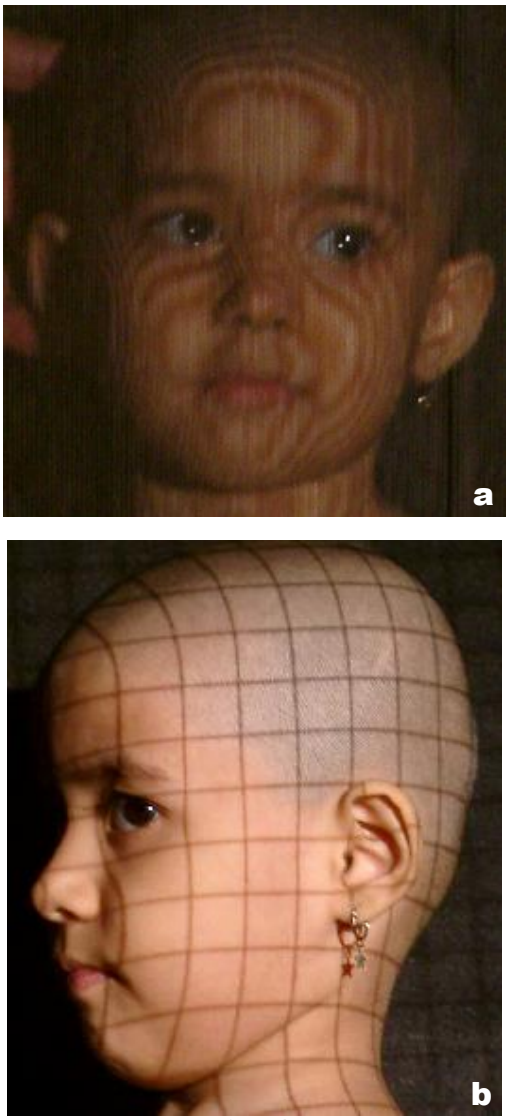

Fig. 4*a*, *b*. Photographs of moiré pattern (top picture) and raster pattern projected on a child's face

Acknowledgments

This work was made possible by Dean's Research Grant awarded by University of Karachi, which is, gratefully, acknowledged. The author would like to thank M. Wasim for drawing resterographic-geometry diagram, Shakeel A. Ansari and Majeed A. Khan for obtaining pictures, using the techniques of moiré fringe topography and rasterstereography, respectively.

Appendix A: Formulae for Height Computation from Moiré Fringe Topographs

a. For shadow type moiré apparatus the distance h_n from the nth fringe to screen (the highest elevation must touch the screen) may be found from [42]**:**

$$h_n = \frac{n\lambda}{d/s_0 - n} \qquad \text{(A1)}$$

where
λ = distance between the camera and the screen
d = distance between the camera and the light source
s_0 = screen interval (line thickness plus spacing)

b. From the above the height difference between successive fringes in a shadow type apparatus may be calculated as [28]:

$$\Delta h = \frac{\lambda d}{s_0[d/s_0 - (n+1)][d/s_0 - n]} \qquad \text{(A2)}$$

For USA studies (1980-82), our group had λ = 100 *cm*, s_0 = 1.0 *mm*, d = 50 *cm*, which gave Δh = 0.20 *cm* for n = 1. For Karachi studies (1988-89), the para-meters were λ = 150 *cm*, s_0 = 1.4 *mm*, d = 110 *cm*, which gave Δh = 0.19 *cm* for n = 1.

c. For the grating hologram type system developed by our group in Karachi, the distance H_n from the nth fringe as compared to the highest elevation is given by:

$$H_n = \frac{nM(M+1)fP_0}{L - nP_0} \qquad \text{(A3)}$$

where
M = magnification of the moiré grid
f = focal length of the projector lens
P_0 = moiré grid interval (line thickness plus spacing)
L = distance between camera and projector lens

The above formula may be obtained by adapting the derivation of Suzuki, Yamashita, Yamaguchi and Armstrong [43] for our system.

d. The height difference between successive fringes for our grating hologram system, therefore, may be expressed as:

$$\Delta H = \frac{M(M+1)fP_0}{L[1-(n+1)M\,P_0/L][1-nM\,P_0/L]} \qquad \text{(A4)}$$

retaining only the linear term in P_0/L ($P_0 \ll L$). Our group used L = 70 *cm* P_0 = 0.0242 *cm*, M = 18.15, f = 8.5 *cm*, which gave ΔH = 1.04 *cm*. The sensitivity may be increased by using finer grid (decreasing P_0) and a lens of shorter focal length. Increasing L may produce distortions.

APPENDIX B: FORMULAE FOR CURVATURE COMPUTATION FROM RASTERSTEREOGRAPHS

Let us suppose that a given raster grid on a plane surface (reference surface) has a periodic spacing equal to s. On the curved surface the spacing appears to be d (Fig. 5). Let the portion of the curved surface under study may be the part of a great circle of radius ρ. Now, we have $s = \rho\phi$, where ϕ is the angle subtended by arc of length s. Therefore

$$\phi = s(\frac{1}{\rho}) = \kappa s \qquad \text{(B1)}$$

Also

$$\begin{aligned} d &= \rho \sin\phi \\ &= \rho(\phi - \frac{1}{3!}\phi^3 + \frac{1}{5!}\phi^5 - .....) \\ &= s(1 - \frac{1}{3!}\kappa^2 s^2 + \frac{1}{5!}\kappa^4 s^4 - ...) \end{aligned} \qquad \text{(B2)}$$

Since ϕ is small we neglect fourth and higher powers. Therefore

$$\frac{d}{s} \approx 1 - \frac{1}{3!}\kappa^2 s^2 \qquad \text{(B3)}$$

which may be put in the form

$$\kappa = \pm\frac{1}{s}\sqrt{6(1-\frac{d}{s})} \qquad \text{(B4)}$$

If $d = s$, $\kappa = 0$ and we have the condition of a flat surface. Appendices A and B are copied here from [6].

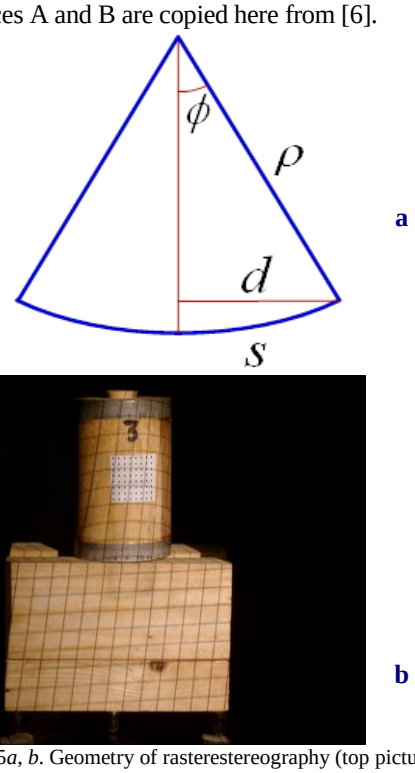

Fig. 5*a*, *b*. Geometry of rasterestereography (top picture) and raster pattern projected on cylinder

REFERENCES

[1] H. R. Lane, "Photogrammetry in medicine," *Photog. Eng.*, vol. 49, pp. 1453-1456, 1983

[2] S. A. Kamal, "3-D optical imaging and image processing: biomedical applications," *Proceedings of the InternationalWorkshop on Recent Advances in Computer Vision*, J. R. Laghari, A. A. Naqvi, A. Q. Rajput, N. A. Sangi and M. A. Shah, Eds. Karachi: SZABIST, 1998, pp. 86–95

[3] H. Takasaki, "Moiré topography," *Appl. Optics*, vol. 4, pp. 845-850, 1970

[4] H. Takasaki, "Moiré topography," *Appl. Optics*, vol. 9, pp. 1457-1462, 1973 [5] Y. A. Siddiqui, and A. S. Choudhry, "Gait analysis using moiré fringe topography and rasterstereography," *M. Sc. Project*, 1990, University of Karachi (unpublished)

[6] S. A. Kamal, A. S. Choudhry and Y. A. Siddiqui, "Gait analysis using moiré fringe topography and rasterstereography (simultaneous recording)," *Kar. U. J. Sc.*, vol. 24, pp. 7-18, 1996

[7] S. A. Kamal, "Combination of moiré contours and edge-based algorithm to study motion in the sagittal plane," *Kar. U. J. Sc.* vol. 24, pp. 53-60, 1996

[8] S. A. Kamal, Naseeruddin and M. Waseem, "Physics of the screening procedures to detect trunk deformities," *3rd Annual Symposium of the Aga Khan University - Impact of Research on Health, Education and Community Development*, Karachi, p. 115, September 1996

[9] M. Akram and S. A. Kamal, "Role of moiré fringe topography in the skeletal examination of school athlete," *International Congress & Exposition on Sports Medicine and Human Performance*, Vancouver, Canada, 1981

[10] M. M. El-Sayyad and S. A. Kamal, "The use of holographic techniques to obtain moiré topographic fringes of the human body," *Bull. Amer. Phys. Soc.*, vol. 27, p. 502, 1982

[11] S. A. Kamal and M. A. K. Yosufzai, (1979) "Moiré contour recorder," *19th Annual Science Conference*, Quaid-e-Azam University, Islamabad, Pakistan, 1979

[12] J. A. Zubairi, "Image-processing algorithms to detect trunk deformities," *New IT Order, Proceedings of XIII Conference of South East Asia Regional Computer Confederation*, pp. 270-279, November 1994

[13] I. V. Adair, M. C. van Wijk and G. W. D. Armstrong, "Moiré topography in scoliosis screening," *Clin. Orthop.*, vol. 129, pp. 165-171, 1977

[14] S. Willner, "Moiré topography for the diagnosis and the documentation of scoliosis," *Acta . Orthop. Scand.*, vol. 50, pp. 295-302, 1979 1981

[15] S. A. Kamal and M. M. El-Sayyad, "The use of moiré topographs for the detection of orthopedic defects in children of age group four-to-seven years," *23rd Annual Meeting of the American Association of Physicists in Medicine*, Boston, Ma., U. S. A.; *Med. Phys. (USA)* vol.8, p.549, 1981

[16] S. A. Kamal, Naseeruddin, M. Waseem and S. Firdous, "Physics of scoliosis screening in school -going children," *Kar. U. J. Sc.*, vol. 26, pp. 5-12, 1988

[17] S. A. Kamal, "Moiré topography," *Physics Dialogue (Karachi)*, vol. 1, pp. 16-17, 1988

[18] S. A. Kamal, "Moiré fringe topography to detect scoliosis in children," *the News International*, Karachi, Pakistan, Technotalk Page, August 11, 1997

[19] B. Ahmad and U. F. Hashmi, "To develop different techniques to study spinal deformity," *M. Sc. Project*, University of Karachi (unpublished), 1990

[20] S. A. Kamal, N. Bukhari, and M. Akram, "A comparison of back moiré topographs of children in sitting and standing positions," *Surface Topography and Body Deformity* (Proceedings of the 5th International Symposium, Vienna, Austria, September 1988), H. Neugebauer and G. Windischbauer, Eds. Stuttgart and New York: Gustav Fischer, 1990, pp. 77, 78

[21] S. A. Kamal, N. Bukhari, and M. Akram, "A comparison of side moiré topographs of children in sitting and standing positions," *Surface Topography and Body Deformity* (Proceedings of the 5th International Symposium, Vienna, Austria, Sep-Tember 1988), H. Neugebauer and G. Windischbauer, Eds. Stuttgart and New York: Gustav Fischer, 1990, pp. 79, 80

[22] M. M. El-Sayyad and S. A. Kamal, "Cobb's angle measurement by moiré topographs," *Proc. 34th Ann. Conf. Eng. Med. Biol. (USA)*, vol. 23, p. 311, 1981

[23] S. A. Kamal, "Measurement of the angle of spinal curvature by moiré topographs," *J. Islamic Med. Assoc. (USA)*, vol. 14, pp. 146-148, 1982

[24] S. A. Kamal, "Moiré topography for the measurement of angle of spinal curvature in three dimensions," *Bull. Amer. Phys. Soc.*, vol. 27, p. 301, 1982

[25] S. A. Kamal, "Determination of degree of correction of spinal deformity by moiré topographs," *Moiré Fringe Topography and Spinal Deformity* (Proceedings of the 2nd International Symposium, Münster, Germany, September 1982), B. Drerup, W. Frobin and E. Hierholzer, Eds. Stuttgart and New York: Gustav Fischer, 1983, pp. 117-126

[26] S. A. Kamal, "Moiré fringe topography and spinal deformity," *National Guard 8th Saudi Medical Conference*, Riyadh, Saudi Arabia, October-November 1983

[27] S. A. Kamal, "Moiré topography for the study of multiple curves of spine," *Surface Topography and*

Spinal Deformity (Proceedings of the 4th International Symposium, Mont Sainte Marie, Québec, Canada, 1986), I. A. F. Stokes, J. R. Pekelsky and M. S. Moreland, Eds. Stuttgart and New York: Gustav Fischer, 1987, pp. 43-50

[28] S. A. Kamal and R. E. Lindseth, "Moiré topography for the detection of orthopedic defects," *Periodic Structures, Moiré Patterns and Diffraction Phenomena*, Proc. Soc. Photo-Opt. Instr. Eng., San Diego, U. S. A., vol. 240, pp. 293-295, 1980

[29] M. Nissinen, M. Heliovaara, J. Seitsamo and M. Poussa, "Trunk asymmetry, posture, growth, and risk of scoliosis: a three-year follow-up of Finnish prepubertal school children," *Spine* vol. 18, pp. 8-13, 1993

[30] M. A. K. Yosufzai, S. A. Kamal and J. A. Zubairi, "Computer-based analysis of human gait using moiré fringe topography," *Proc. 2nd Int. Workshop on Computer Vision and Parallel Processing*, G. N. Khan, A. A. Naqvi and M. Shah, Eds. Quaid-é-Azam University, pp. 60-71, January 1995

[31] S. A. Kamal, M. Akram and N. Bukhari, "Moiré topography for the study of neurological disorders," *2nd National Symposium on Frontiers in Physics*, Quaid-e-Azam University, Islamabad, Pakistan, 1988

[32] S. A. Kamal, M. Akram, K. A. Siddiqui, and N. U. Khan, "Moiré, raster & EEG studies of epileptics during the washable-memory period," *7th International Conference on Biomagnetism*, New York University, New York, U. S. A., August 1989

[33] M. Akram, "Construction of a shadow type moiré apparatus," *M. Sc. Project*, University of Karachi (unpublished), 1989

[34] S. A. Kamal, "Reproducibility of moiré topographs," *Surface Topography and Body Deformity* (Proc. 5th Int. Symp.), loc. cit., pp.151-153

[35] S. A. Kamal, G. Bennoni and S. Willner, "A study to test the reproducibility of moiré topographs," *Kar. U. J. Sc.*, vol. 22, pp. 67-74, 1994

[36] M. Van Wijk, "Moiré contourograph --- an accuracy analysis," *J. Biomech.*, vol. 13, pp. 605-613, 1980

[37] M. Van Wijk, "Accuracy of moiré topography," *Moiré Fringe Topography and Spinal Deformity*, (Proceedings of the 1st International Symposium, Basin Harbor, Vermont, U. S. A., 1979), M. S. Moreland, M. H. Pope and G. W. D. Armstrong, Eds. New York: Pergamonn, 1981, pp. 47-57

[38] Naseeruddin, S. A. Kamal and S. Firdous, "Accuracy and precision of moiré fringe topography system," *Pakistan Institute of Physics International Conference*, March-April 1997, Lahore, Pakistan

[39] T. Lauland, J. O. Søjbjerg and E. Hørivck, "Moiré topography in school screening for structural scoliosis," *Acta Orthop Scand.*, vol. 3, pp. 765-8, 1982

[40] S. A. Kamal, "A new process for patient alignment," *Bull. Amer. Phys. Soc.*, vol. 27, p. 502, 1982

[41] K. Stüben, "Multigrid strategies - applications and techniques," *17th International Nathiagali Summer College on Physics and Contemporary Needs*, Nathiagali, Pakistan, June-July 1992

[42] H. Takasaki, "The development and the present status of moiré topography," *Holography in Medicine and Biology* (Proceedings of the International Workshop, Münster, Germany), Ed. G. von Bally, Berlin, Heidelberg and New York: Springer, 1979, pp. 45-59

[43] N. Suzuki, Y. Yamashita, Y. Yamaguchi and G. W. D. Armstrong, (1981) "Measurement of posture using moiré topography," *Moiré Fringe Topography and Spinal Deformity* (Proc. 1st Int. Symp.), loc. cit., pp. 121-131

Web address of this document (*author's homepage*)**:** http://www.ngds-ku.org/Papers/C68.pdf
*Abstract***:** http://www.ngds-ku.org/pub/confabst.htm#C68:

1-4244-2427-6/08/$20.00 ©2008 IEEE